

FREND™ System

# FREND™ 2.0

## User manual



FRENDS™ System,  
**FRENDS™ 2.0 User Manual**

**Thank you for purchasing the FRENDS™ 2.0.**

Please take a few minutes to read this user manual.

If you have any question, please contact NanoEntek, Inc.

Customer support.

Tel: +82-2-6220-7940

Fax: +82-2-6220-7999

E-mail: ivdst@nanoentek.com

This manual is considered a necessary part of the device: It must be available for the operator to use at the bench as well as for the individual responsible for instrument maintenance.



**NanoEntek, Inc.**

851-14, Seohae-ro, Paltan-myeon, Hwaseong-si, Gyeonggi-do, 18531, Korea

Tel: +82-2-6220-7940

Fax: +82-2-6220-7999

Copyright © 2025 NanoEntek, Inc.

All right reserved. Published in Korea

Document number: **NESMU-F20-001EN**

Revision history: **V.0.0 MAY 2025**

The contents of this user manual are subject to Korean and International copyright laws, affording them legal protection. Any form of reproduction, translation, publication, or distribution of these materials without explicit permission from the copyright owner is strictly prohibited.

# Table of Contents

<b>Introduction .....</b>	<b>4</b>
Warranty .....	4
Introduction .....	5
Intended use .....	6
Product Components.....	7
Safety symbols & abbreviations.....	8
General safety warnings.....	11
FRENDD™ 2.0 Description.....	13
Functions of Codechip and associated cartridge .....	14
Software keys .....	15
 <b>Setup .....</b>	 <b>28</b>
FRENDD™ 2.0 Setup procedure .....	28
 <b>Operation .....</b>	 <b>33</b>
FRENDD™ 2.0 Operating procedure .....	33
FRENDD™ 2.0 Data management .....	38
 <b>Maintenance .....</b>	 <b>40</b>
FRENDD™ 2.0 Maintenance .....	40
FRENDD™ 2.0 Update.....	44
Cleaning and storage .....	45
Trouble-shooting .....	46
General specification - normal environmental conditions .....	49
Customer support information .....	50

# Introduction

## Warranty

NanoEntek Inc. warranties the original purchaser for one (1) year from the date of its initial purchase that this device and other devices sold by one of its authorized representatives will function as specified.

NanoEntek Inc. and its representatives shall be relieved of any liability under this warranty if the product is not used in accordance with the manufacturer's instructions, altered in any way not specified by NanoEntek Inc., not regularly maintained, used with device not approved by NanoEntek, Inc. or used for purposes for which it was not designed.

This warranty does not apply to damages incurred during the initial shipment of the instrument and associated auxiliary materials. Any damages incurred on initial shipment are to be reported immediately to the freight carrier for the settlement of the claim. Please examine the device carefully for any damage before signing for the shipment since your signature indicates receipt of undamaged device.

NanoEntek Inc. will not be responsible for any indirect, incidental, special, consequential or punitive damages or other losses, including, but not limited to, damages to or losses of other properties or device.

NanoEntek will not be responsible for personal injuries, whether to the purchaser or others.

# Introduction

## Introduction

## The principle of the FREND™ System, FREND™ 2.0


The FREND™ System, FREND™ 2.0 is a portable, automated FREND™ cartridge reader.

The FREND™ System, FREND™ 2.0 is based on quantitative and qualitative immunoassay technology capable of quantifying single or multiple analytes by measuring laser-induced fluorescence in a single-use disposable reagent cartridge.

The FREND™ System, FREND™ 2.0 is a Class 1 laser product in accordance with IEC 60825-1:2014.

The FREND™ cartridge utilizes micro-fluidics lateral flow technology where the analyte of interest in the sample forms immune complexes while moving through the fluidics pathway in the cartridge.

The concentration of the analyte of interest in an unknown sample is calculated using the ratio of the fluorescent intensity of the test zone and the reference zone.

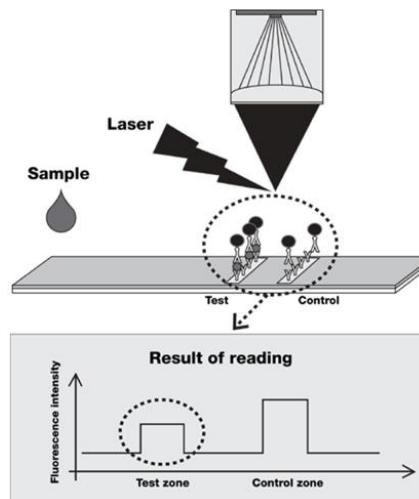

The principle of the fluorescence detection and calculation of the analyte concentration (drawing from the manual).

# Introduction

## Intended use

The FREND™ System, FREND™ 2.0 is designed to accommodate the FREND™ cartridge, which helps in clinical management of patients by quantitatively or qualitatively measuring or diagnosing specific antigen or antibodies *in vitro* in human specimens.

# Introduction

## Product Components

When the FREND™ System, FREND™ 2.0 is received, open the shipping box and carefully check the package contents. Note that the Q.C. designation is used in terms of hardware verification of performance not quality control of the actual testing process for any analytes.

**Main Device**




**Adaptor/Power Cord**



**Pipette**




**QC Cartridge**




**QC Code chip**



**USB Drive**



**Tube rack**



**User Manual**



**Quick Manual**



# Introduction

## Safety symbols & abbreviations

Following symbols are found on the FREND™ System, FREND™ 2.0 user manual and FREND™ cartridge package inserts. Please note the meanings of the symbols and always use the device in a safe manner.

Symbol	Definition
	Caution, Warning, Consult accompanying documents
	Catalogue number/Reference number
 www.nanotek.com	Consult Instructions for Use An electronic instructions-for-use (eIFU) indicator (website address) may accompany the symbol when used to indicate an instruction to consult an eIFU.
	Serial number
	Manufacturer
	Date of Manufacturer
	General symbol for recover/recyclable
	CE marking
	UK Conformity Assessment
	In vitro diagnostic medical device
	Class I laser product
	Electrical rating
	Electrical input
	Biohazard
	Meets FCC requirements per 21 CFR Part 15 This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference in which case the user will be required to correct the interference at his own expense.

# Introduction

## Safety symbols & abbreviations

Symbol

## Definition

### Dimensions

This product conforms to UL 61010-1, CAN/CSA C22.2 No.61010-1 "Safety Requirements for Electrical Equipment for Measurement, Control, and Laboratory Use, Part 1: General Requirements." Instruments bearing the TUV symbol are certified by TUV Products Services to be in conformance with the applicable safety standard for the US and Canada.

### Gross weight

### Storage temperature

### Storage Humidity

For prescription use only  
CAUTION: Federal (The U.S.) law restricts this device to sale by or on order of a physician.

### This way up

### Disposal of your old appliance

1. When this crossed-out wheeled bin symbol is attached to a product, it means the product is covered by the European Directive 2012/19/EU.
2. All electrical and electronic products should be disposed of separately from the municipal waste stream via designated collection facilities appointed by the government or the local authorities.
3. The correct disposal of your old appliance will help prevent potential negative consequences for the environment and human health.
4. For more detailed information about disposal of your old appliance, please contact local distributor, waste disposal service or call the number listed in the manual.

Keep dry  
keep away from rain

Fragile, handle with care

US Corporation

European Corporation

Authorized representative in the European Community

Authorized representative in United Kingdom

Authorized representative in Switzerland

Authorized representative in Brazil

# Introduction

## Safety precautions

Thoroughly read all instructions before attempting to operate this device. Pay particular attention to all safety precautions. The following guidelines must be observed during every phase of operation. Breaking these rules may be dangerous, illegal or affect performance of the device and/or invalidate the device approval and/or warranty. In order to avoid instrument damage or personal harm, read this manual carefully and follow the instructions given.

- Always ensure that the power supply input voltage matches the voltage available in your location.
- This machine is air-cooled so its surface becomes warm during operation.
- When installing the device on the countertop always leave a space of more than 10 cm (4 inches) around the instrument in all directions.
- Leave adequate distance between the back of the instrument and the wall to allow the operation of the 'on' and 'off' power button.
- This location must also be accessible to load the Q.C. Code chip and the test code chips.
- Do not insert metallic objects into the FREND™ 2.0 as this could result in an electrical shock, personal injury and device damage.
- Insert only qualified and authorized devices supplied by NanoEntek Inc.
- Do not insert any foreign materials into the ventilation.
- Always set the main switch to the 'off' position before connecting the power cord to the wall outlet.
- When unplugging the power cord, be certain to turn off the device, then unplug the power cord.

**NOTE:** This device has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference when the device is operated in a commercial environment. This device generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this device in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

# Introduction

## General safety warnings

- Before using the device, read this manual and be certain you thoroughly understand its contents.
- Please follow the instructions in this manual to assure proper operation of the device.
- When not in use, unplug the device from the electrical outlet.
- Perform regular maintenance checks on the main body of the instrument.
- Inspect all the components.
- After long term storage, take extra care to be sure the device operates correctly.
- Avoid handling or storing liquid on or near the device.
- Do not open the machine at any time while it is operating or when it is plugged in to the wall outlet.
- Keep the instrument away from open flames and or smoke.
- When moving the device, unplug it and move it carefully and gently.
- The instrument should be placed on a flat and stable surface.
- Refer to this manual for handling and/or maintenance.
- Keep the device (including the cable and the plug) out of reach of children.
- Disposal management.
- Place the device in a location accessible only to authorized personnel to prevent use by unauthorized individuals.

---

Local regulations governing the disposal of materials containing biohazardous materials must be observed. It is in the responsibility of the user to arrange for the proper disposal of these items.

---

All instrument parts which may be contaminated with potentially infectious materials must be disinfected by suitable validated procedures (autoclaving, chemical treatment) prior to disposal if this is required by the regulations under which your site operates.

---

The device itself and the electronic accessories must be disposed of according to the regulations for the disposal of electronic components. Be sure to understand what the rules at your site are.

---

# Introduction

## General safety warnings

- Do not attempt to disassemble/modify the device.
- Do not insert foreign objects into the device and insert only NanoEntek Inc. provided cartridges.
- Do not handle the device or the power cord with wet hands.
- Do not move, tilt, jar or shake the device when it is in operation.
- Do not store the device in direct sunlight, high/low temperatures or high humidity.
- Do not throw, drop, hit or push the device.
- Do not touch the device or the plug during an active thunder and/or lightning storm.
- Do not touch the LCD panel with sharp objects.
- Do not use the device, if it has any damaged parts (including the power cord or the plug).
- Do not look into the cartridge slot so that your eyes are not exposed to the laser.

Caution - Use of controls or adjustments or performance of procedures other than those specified herein may result in hazardous radiation exposure



Warning  
or caution

There is a risk of explosion, if the instrument battery is replaced with an incorrect type.

Class A device is intended for use in an industrial environment. In the documentation for the user, a statement shall be included drawing attention to the fact that there may be potential difficulties in ensuring electromagnetic compatibility in other environments, due to conducted as well as radiated electromagnetic disturbances from the instrument itself.



Biohazard

The cartridge should be inserted into the device within the stipulated time.

The instrument should be used in a clean environment.


Ensure the sample is not contaminated by any foreign material or contain fibrin clots.

Human samples and controls should be considered potentially infectious.

# Introduction

## FREND™ 2.0 Description

Name	Function
Screen	Show the operating status and results
Cartridge slot	Slot for FREND™ cartridge insertion and ejection
Power button	Power on/off
USB port	Use to connect to a USB drive.
Code chip slot	Slot for QC or cartridge Code chip insertion and ejection
Barcode reader	Read the QR code or barcode information
Power supply port	Power supply
Thermal printer	Print the result

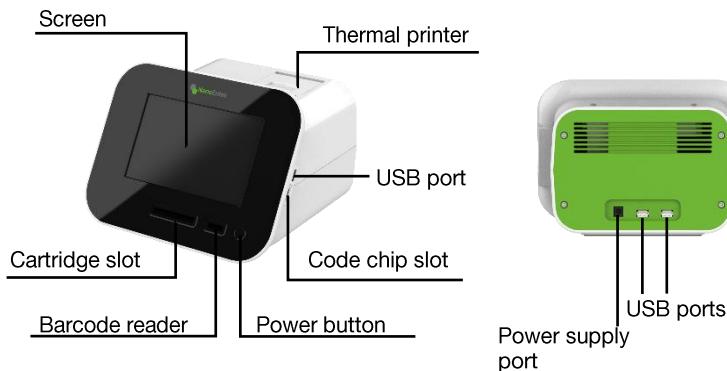

# Introduction

## Functions of Code chip and associated cartridge

Product	Definition
QC Code chip	The chip containing information for the proper functioning of the QC Cartridge
QC Cartridge	The cartridge used to check the mechanics and optics of the FREND™ 2.0.
Product	Definition
Code chip	This cartridge code chip is specific for a given analyte and lot of reagents. It contains information on calibration and calculation of results using readings from the FREND™ reagent cartridge
FREND™ cartridge	The cartridge contains reagents and microstructures to support a lateral flow assay, where analytes of interest from immune complexes while the specimen is moving and being separated. Ratio between test zone and reference zone is calculated.

# Introduction

## Software keys

### Login screen

**Login**

User ID

Password

**Login**




Button	Purpose
User ID	Pre-registered user ID required for login
Password	Pre-registered user password required for login
	Delete the entered information
<b>Login</b>	Login to the main page after entering all the user information

# Introduction

## Software keys

### Main screen

**FREND™ 2.0**

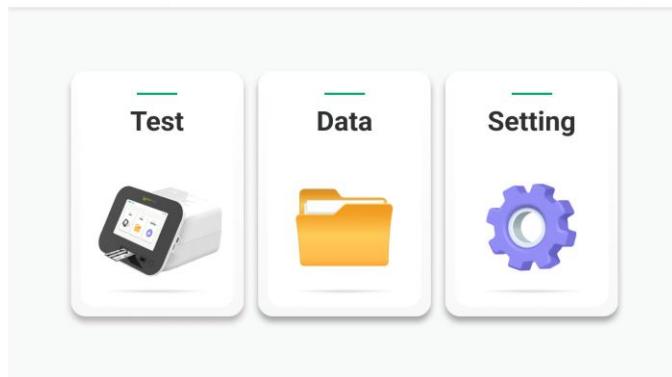


Button	Purpose
	Initiate a test sequence for specimens or maintenance using that analyte-specific cartridge or QC cartridge
	Check and search results. Back up the data and transfer the data to a USB drive or LIS/HIS.
	Set up the parameters specific to the site and operator
	Notification <ul style="list-style-type: none"><li>- Data storage status</li><li>- FREND™ cartridge expiry date</li></ul>
	User <ul style="list-style-type: none"><li>- Logout from the system</li></ul>

# Introduction

## Software keys

### Test screen

FRENDS™ 2.0

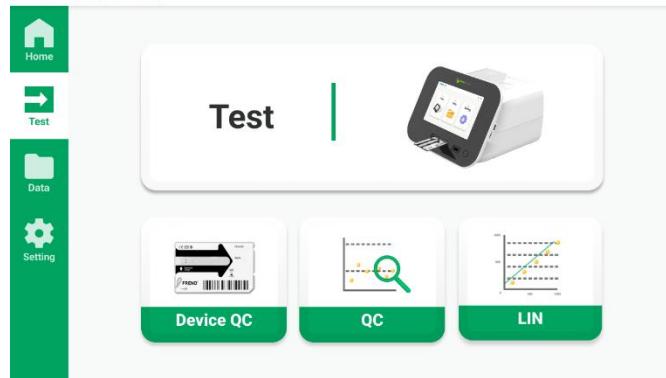

Button	Purpose
	Run the specimens of the patient on the FRENDS™ cartridge
	Access the device functions with QC cartridge
	Verify the FRENDS™ cartridge with the external or internal QC materials (Optional) <small>*Internal or external quality control materials are required</small>
	Verify the FRENDS™ cartridge with the linearity or verification kit (Optional) <small>*External verification materials are required</small>


### \*Navigation Bar

	Navigate to Home screen
	Move to Test screen for testing specimens or maintenance
	Access the Data screen to manage the recorded data
	Access the Setting screen to check device information

# Introduction

## Software keys

### Test screen » Information input

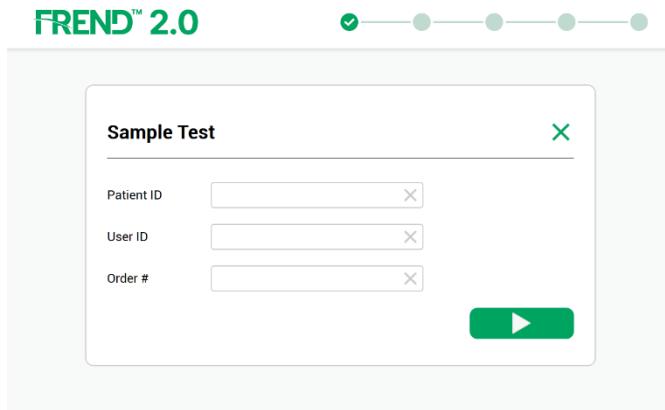


Button	Purpose
Patient ID	Enter the patient identifying information
User ID	Select a pre-registered or enter a new user name
Order #	Type the patient identifying number or additional information (Optional)
	Start the test after entering information
	Cancel the test and move to the previous screen

# Introduction

## Software keys

### Data screen

FRENDS™ 2.0

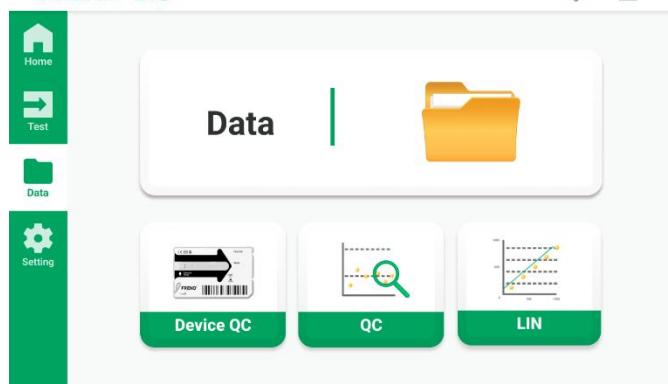


Button	Purpose
	Review recorded patient results
	Check device performance confirmed with the QC cartridge.
	Access the product performance validated with quality control materials.
	Verify the linearity/calibration verification results on the product

# Introduction

## Software keys

### Data screen

**FRENDS™ 2.0**

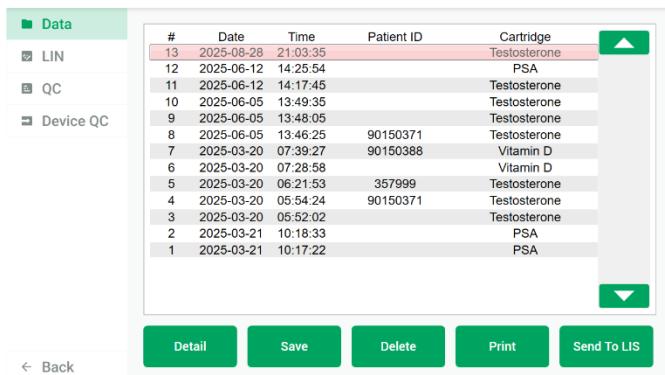

#	Date	Time	Patient ID	Cartridge
13	2025-08-28	21:03:35		Testosterone
12	2025-06-12	14:25:54		PSA
11	2025-06-12	14:17:45		Testosterone
10	2025-06-05	13:49:35		Testosterone
9	2025-06-05	13:48:05		Testosterone
8	2025-06-05	13:46:25	90150371	Testosterone
7	2025-03-20	07:39:27	90150388	Vitamin D
6	2025-03-20	07:28:58		Vitamin D
5	2025-03-20	06:21:53	357999	Testosterone
4	2025-03-20	05:54:24	90150371	Testosterone
3	2025-03-20	05:52:02		Testosterone
2	2025-03-21	10:18:33		PSA
1	2025-03-21	10:17:22		PSA

**Buttons:**

- Detail
- Save
- Delete
- Print
- Send To LIS

[← Back](#)

Button	Purpose
Detail	Review the recorded details
Save	Save the data to the flash drive connected to USB port
Delete	Delete the selected data
Print	Print the chosen data
Send to LIS	Transfer the selected data to the information system in the laboratory or hospital.

### \*Navigation Bar


<b>■ Data</b>	Review recorded patient results
<b>■ LIN</b>	Verify the linearity/calibration verification results on the product
<b>■ QC</b>	Access the product performance validated with quality control materials.
<b>■ Device QC</b>	Check device performance confirmed with the QC cartridge

# Introduction

## Software keys

### Setting screen

FRENDS™ 2.0

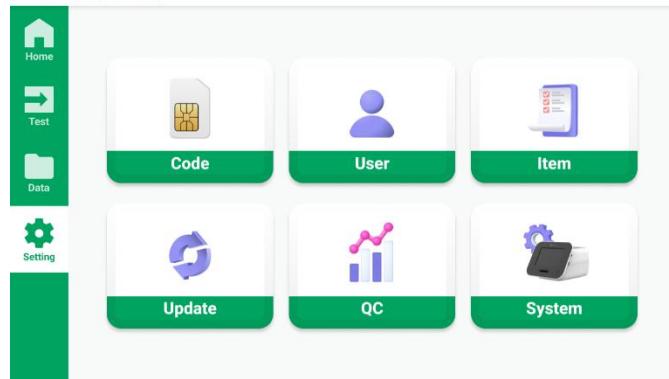


Button	Purpose
	Register the cartridge information using code chip or QR code
	User information registration and management
	View the registered cartridge list and manage the details
	Update the software
	Register and manage the QC and Linearity kit information
	Manage and set the device information · Information: Region/Language, S/N, S/W and F/W version · Date & Time · Test Option: Quick mode, Requirement, Lab ID · Device: Sound, LIS setting, DB Reset, System Log

# Introduction

## Software keys

### Setting screen » Codechip

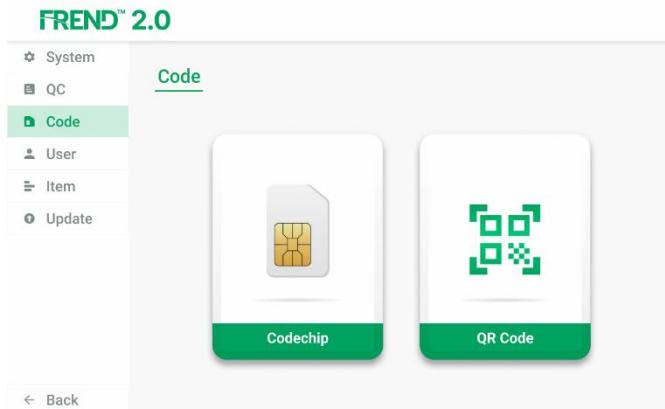

Button	Purpose
	Install using the codechip
	Scan the QR Code to save cartridge information
<a href="#">← Back</a>	Move to the previous screen

*Navigation Bar	
	System Manage and set the device information
	QC Register and manage the QC and Linearity kit information
	Code Register the cartridge information through code chip or QR code
	User Manage the user information
	Item View the registered cartridge information and input the normal range
	Update Update Software

# Introduction

## Software keys

### Setting screen » User

FRENDS™ 2.0

System  
QC  
Code  
**User**  
Item  
Update

#### User

#	User ID	First Name	Last Name
1	master		master
2	user1	Ellen	Jang
3	user2	Steve	Jung

New

Delete

Edit

← Back

Button	Purpose
New	Register the user information
Delete	Remove the user information
Edit	Edit the user information
← Back	Move to the previous screen

# Introduction

Software  
keys

Setting screen » Item

**FREND™ 2.0**

System  
QC  
Code  
User  
**Item**  
Update

Code chip	Options	
LOT 303009	EXP Date 2026-12-31	Installed Date 2025-03-13
303020	2026-07-01	2025-03-13
303080	2026-12-31	2025-08-29
303051	2026-07-01	2025-06-12
309999	2026-12-31	2025-08-29

← Back

Button	Purpose
← Back	Move to the previous screen

# Introduction

## Software keys

### Setting screen » QC

#### FRENDS™ 2.0

System

QC

Code

User

Item

Update

QC Linearity Option

#	LOT	EXP Date	Cartridge	Item
1	6360A23002	2024-11-01	Cardiac Triple	Myoglobin
2	6360A23002	2024-11-01	Cardiac Triple	Troponin I
3	6360A23002	2024-11-01	Cardiac Triple	CK - MB
4	1234	2024-01-07	Cardiac Triple	Myoglobin

New

Delete

Edit

Detail

← Back


Button	Purpose
QC	Manage the QC material information
Linearity	Manage the linearity kit information
Option	Enables or disables QC testing on the test screen
New	Register the Cartridge and QC material information.
Delete	Remove the QC material information.
Edit	Edit the QC material information.
Detail	Review the QC material details.
← Back	Move to the previous screen

# Introduction

## Software keys

Setting screen » QC » Option

### FREND™ 2.0

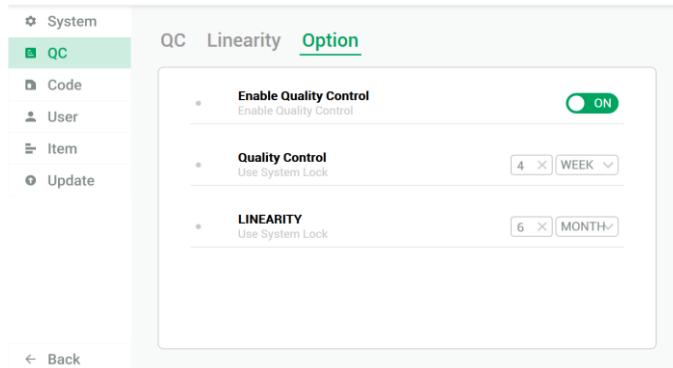

Button	Purpose
Enable Quality Control	Activate / Deactivate the quality control button on the test page
Quality Control Use System Lock	Set the frequency for performing quality control. (Day / Week / Month)
Linearity Use System Lock	Set the frequency for performing Linearity control. (Day / Week / Month)

# Introduction

## Software keys

### Setting screen » System

#### FREND™ 2.0

Information

Region: USA

Language: English

Serial number: F20U250302-002

Software Version: V2.0.0

Firmware Version: V0.1.1

Product Name (Device Name): FREND System (FREND 2.0)

← Back

Button	Purpose
Information	Region selection Language selection System information - Serial number - Software version - Hardware version
Date & Time	Set the system time
Test Option	Set up the following test mode and type the default test information - Quick mode activation / deactivation - Requirement: Patient ID, User ID, Order# - Lab ID
Device	Set the sound volume of the device Set the LIS option Database reset View log in history

# Setup

## FREND™ 2.0 Setup procedure

1. Carefully examine the box for any damage. Remove all the components of the FREND™ 2.0 from the box.

2. Plug the power cord into the adaptor.

3. Carefully examine the adaptor and make certain it is compatible with the power at the plug location.

If it is the appropriate adaptor, plug the adaptor into the FREND™ 2.0 and the AC power cord into the wall socket.



### **Warning:**

If you use an incorrect adaptor, the FREND™ 2.0 may explode or start to burn. If this happens, it will no longer work properly anymore.



4. Press the power button for 3 seconds.

5. While the device is booting up, this image will appear.




# Setup


## FREND™ 2.0

### Setup procedure

#### 6. Log in the system

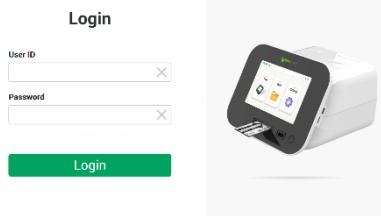

#### 7. Tap the **Setting** button on the main screen.

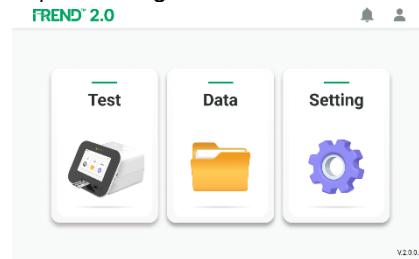


#### 8. Set the **Region** and **Language** on the Information tab

- Supporting site
  - : USA, Korea, Germany, Italy, China, Japan
- Support Language
  - : English, Korean, German, Italian, Chinese, Japanese

#### 9. Tap the **Date & Time** button on the setting screen.

- Set the local date and time

FREND™ 2.0

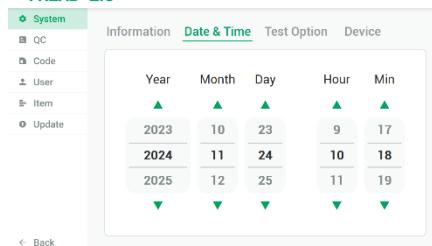

#### 10. After setting the date and time, tap the **Back** button to return to the previous screen.

#### 11. Tap the **Code chip** button.

# Setup

## FRENDS™ 2.0 Setup procedure


### 12. Select the way to install the code chip.

#### - Code chip

- : Insert the QC Code chip into the code chip slot in the direction of the arrow
- : Remove the code chip after the installation

#### - QR code


- : Scan the QR code on the barcode reader

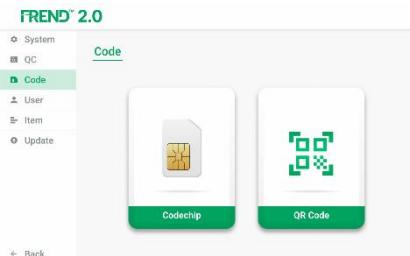

#### **Warning:**

Please check the inserting direction for the QC Code chip. The QC Pouch contains one QC Code chip, which is used with the QC Cartridge to do instrument validation

### 13. The information is on the screen when the QC Code chip installation is complete. Tap the **Back (X)** button to go to the setting screen.

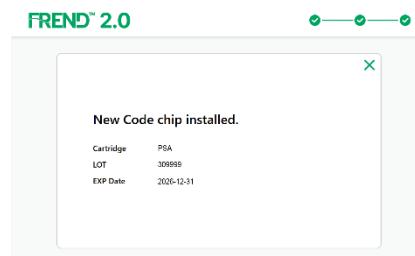

### 14. Tap the **ITEM** button on the setting screen.


### 15. Check the QC Cartridge lot number and the installed date.

# Setup

## FREND™ 2.0 Setup procedure

17. If the QC Code chip installation is complete, tap the **Back** button to go to the main screen.


18. Tap the **TEST** button on the main screen.

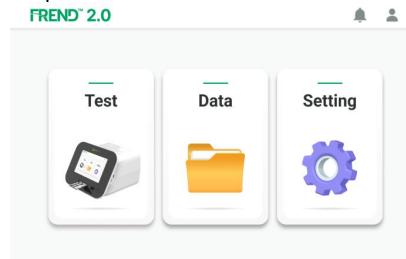

19. Tap the **Device QC** button on the TEST screen.



20. Insert the QC cartridge into the cartridge slot.

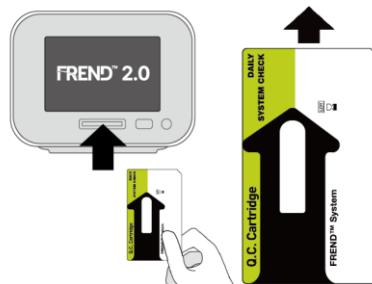


### Warning:

Please check the direction of the QC Cartridge before insertion.

# Setup

## FREND™ 2.0 Setup procedure

21. The QC check which the instrument is operating correctly will complete automatically and the QC Cartridge will be expelled.

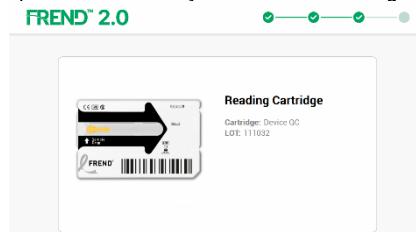

The system automatically checks three steps while reading.

- Step1.** Laser Power
- Step2.** Laser Alignment
- Step3.** Calculate Ratio

22. When the QC check is done, the QC Cartridge automatically emerges and the results from all the three steps are displayed. There will be three Passes, if the system is properly operating.




### Warning:

If all results is not pass, try steps 19-20 again. If the device does not pass all three steps, please contact customer support via email.

23. Tap the **X** button and move to the main screen.

24. Remove the QC Cartridge.

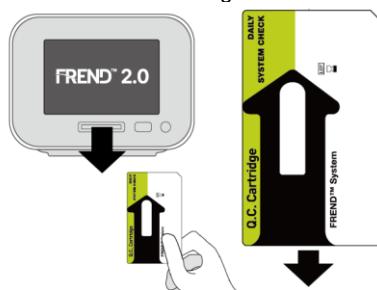

The FREND™ 2.0 setup is complete.

# Operation

## FREND™ 2.0

### Operating procedure


1. Press the power button for 3 seconds.



2. While the device is booting up, this image will appear.



3. Tap the **SETTING** screen on the main screen.

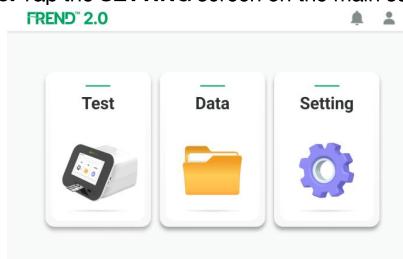

#### Caution:

When installing with a code chip, please double check the direction of the cartridge code chip before insertion. Each cartridge box contains one analyte and lot specific cartridge code chip. The code chip works for all cartridges in the same box.

# Operation

## FREND™ 2.0

### Operating procedure

4. Tap the **Codechip** button.

5. Select the way to install the code chip.


- **Code chip**

- : Insert the QC Code chip into the code chip slot in the direction of the arrow
- : Remove the code chip after the installation

- **QR code**


- : Scan the QR code on the barcode reader

**FREND™ 2.0**

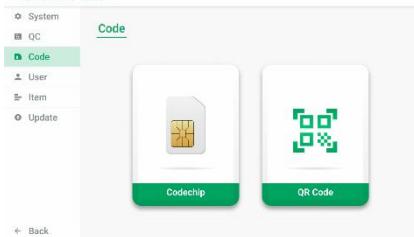

6. When the code chip installation is complete, tap the **Back** button to go to the setting screen.


**FREND™ 2.0**

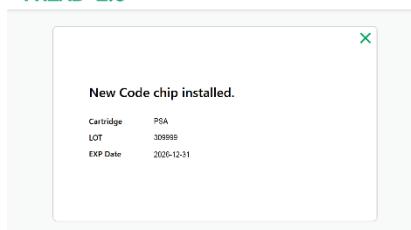

7. Tap the **ITEM** button on the setting screen.

8. Check the cartridge lot number and the installed date.

**FREND™ 2.0**

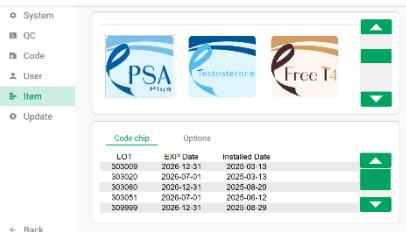

# Operation

## FREND™ 2.0 Operating procedure

9. If the code chip installation is complete, tap the **Back** button to go to the main screen.

10. Prepare the cartridge and patient samples.




- For patient specimens, collect 2-4 mL of blood in a 5 mL tube. An approved blood sample type must be used for each item. Serum and plasma can be separated according to the blood collection tube manufacturer's recommended conditions.


11. After writing the patient information or ID on the sticker of the cartridge, inject sample into the inlet of the cartridge using a calibrated pipette and disposable tip.

**Refer to the package insert for specific sample volume and procedure.**

12. Tap the **TEST** button on the main screen.

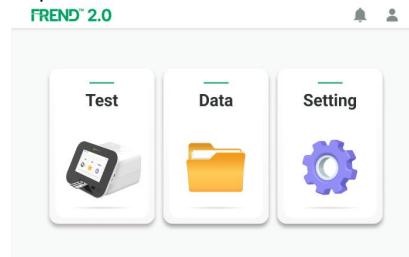

13. Tap the **TEST** button.

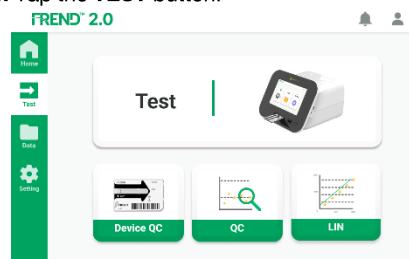


# Operation


## FREND™ 2.0 Operating procedure

- **Test** button is for the patient's specimen testing.
- **Device QC** button is to check the performance of the equipment such as laser power, alignment, and ratio calculation using the QC cartridge
- **QC** button is to check the performance of the cartridge with internal or external quality control material.
- **LIN** button is to check the performance of the cartridge with the linearity kit. \*the USA only

14. Type the 'Patient ID', and 'Order #' and select the 'User ID'. Tap the Enter button. To start a test, tap the **NEXT(▶)** button.

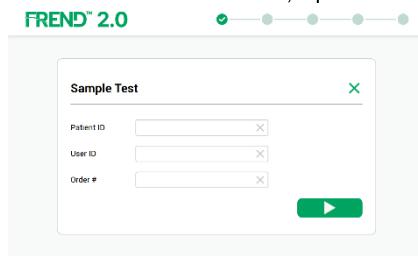

15. Insert the cartridge into the cartridge slot.

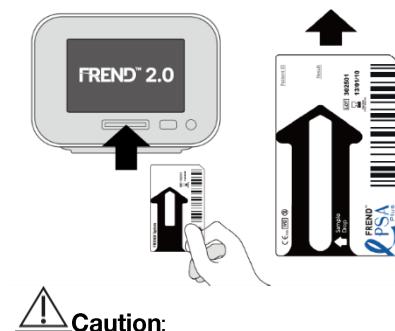

### Caution:


Please check the direction of the cartridge before insertion. And also check if the insertion is complete.

# Operation


## FREND™ 2.0 Operating procedure

**17.** Wait until the test is done automatically. After the reaction is complete, the FREND™ 2.0 starts to record the fluorescent readings.

\* If you cancel the test, please tap the **X** button on the screen.

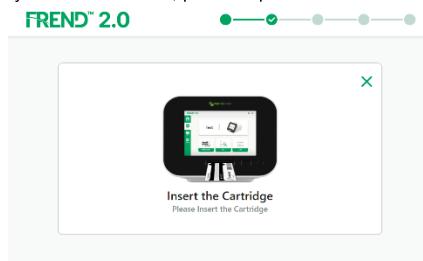

**18.** When the test is done, the cartridge is expelled and the result is displayed on the screen.

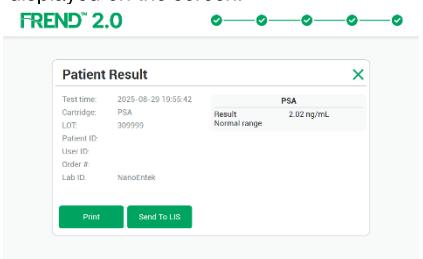

\* Print the result by tapping the **PRINT** button.

\* Tap the **Send to LIS** button to transfer the data to the management system in the clinic

**19.** The test is complete. If another sample is to be run, repeat again steps 34 - 36.

- The results are stored automatically. If the **DATA** button on the main screen is tapped, more information is visible.

# Operation

## FREND™ 2.0 Data management

Tap the **DATA** button on the main screen to check, delete, and perform data backup.


### Data selection

FREND™ 2.0

#	Date	Time	Patient ID	Cartridge
7	2025-03-20	07:39:27	90150388	Vitamin D
6	2025-03-20	07:28:56		Vitamin D
5	2025-03-20	06:58:53	367999	Testosterone
4	2025-03-20	05:54:24	90150371	Testosterone
3	2025-03-20	05:52:02		Testosterone
2	2025-03-21	10:18:33	PSA	PSA
1	2025-03-21	10:17:22		PSA

Drag the screen up or down to check the data. You can select the desired data by tapping the list.

### Data backup

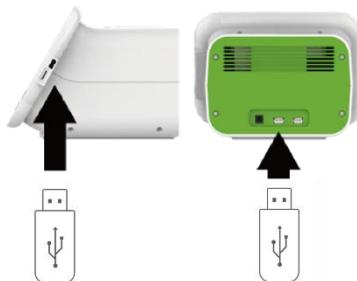

Connect the USB drive that will receive the data backup to a USB port on the side and back of the device.

FREND™ 2.0

#	Date	Time	Patient ID	Cartridge
7	2025-03-20	07:39:27	90150388	Vitamin D
6	2025-03-20	07:28:56		Vitamin D
5	2025-03-20	06:58:53	367999	Testosterone
4	2025-03-20	05:54:24	90150371	Testosterone
3	2025-03-20	05:52:02		Testosterone
2	2025-03-21	10:18:33	PSA	PSA
1	2025-03-21	10:17:22		PSA


Tap the **Save** button to store all data on the USB drive.

# Operation

## FRENDS™ 2.0 Data management

### Data print

FRENDS™ 2.0

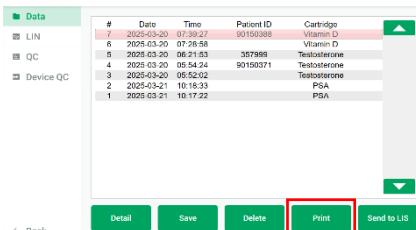

■ Data


#	Date	Time	Patient ID	Cartridge
7	2025-03-20	07:39:27	90150388	Vitamin D
6	2025-03-20	07:26:58		Vitamin D
5	2025-03-20	06:21:53	357999	Testosterone
4	2025-03-20	05:54:24	90150371	Testosterone
3	2025-03-20	05:52:02		Testosterone
2	2025-03-21	10:18:33		PSA
1	2025-03-21	10:17:22		PSA

Detail Save Delete Print Send to LIS

Tap the **PRINT** button to be printed the selected data from the built-in Print.

### Data transfer to LIS

FRENDS™ 2.0

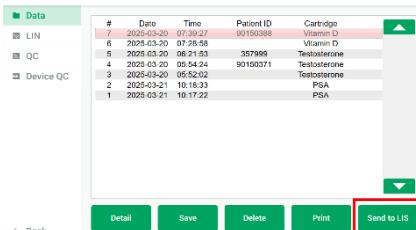

■ Data


#	Date	Time	Patient ID	Cartridge
7	2025-03-20	07:39:27	90150388	Vitamin D
6	2025-03-20	07:26:58		Vitamin D
5	2025-03-20	06:21:53	357999	Testosterone
4	2025-03-20	05:54:24	90150371	Testosterone
3	2025-03-20	05:52:02		Testosterone
2	2025-03-21	10:18:33		PSA
1	2025-03-21	10:17:22		PSA

Detail Save Delete Print Send to LIS

Tap the **Send to LIS** button for sending the selected data to the connected LIS.

### Data deletion

FRENDS™ 2.0

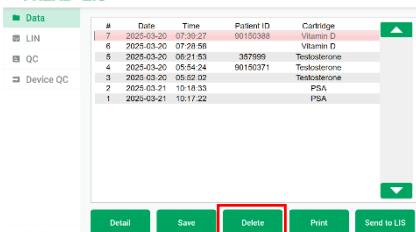

■ Data

#	Date	Time	Patient ID	Cartridge
7	2025-03-20	07:39:27	90150388	Vitamin D
6	2025-03-20	07:26:58		Vitamin D
5	2025-03-20	06:21:53	357999	Testosterone
4	2025-03-20	05:54:24	90150371	Testosterone
3	2025-03-20	05:52:02		Testosterone
2	2025-03-21	10:18:33		PSA
1	2025-03-21	10:17:22		PSA

Detail Save Delete Print Send to LIS

The chosen data can be removed from tap the **DELETE** button.

# Maintenance

## FREND™ 2.0 Maintenance


### The FREND™ 2.0 checks

To assure reliable and accurate test results, please check the following:

- Observe the external appearance and screen of the FREND™ 2.0 every time you use the device.
- Start by scrutinizing the signal input section of the FREND™ 2.0 on a monthly basis, irrespective of device usage. Employ the QC Cartridge and the QC code chip to conduct precise optical testing.
- Halt device usage immediately and reach out to the supplier's customer support if any issues are detected in the results following the checkup.

### The FREND™ 2.0 maintenance supplies

#### QC Cartridge



#### QC Code Chip



### The FREND™ 2.0 checklist are:

1. Laser Power
2. Laser Alignment
3. Calculate Ratio


# Maintenance

## FREND™ 2.0 Maintenance

1. Press the power button for 3 seconds.



2. Tap the **SETTING** button on the main screen.
3. Tap the **Codechip** button.
4. Select the way to install the code chip.
  - **Code chip**
    - : Insert the QC Code chip into the code chip slot in the direction of the arrow
    - : Remove the code chip after the installation
  - **QR code**
    - : Scan the QR code on the barcode reader

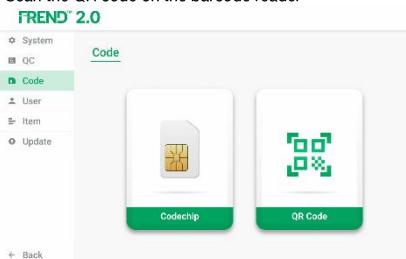


### **Warning:**

Please check the inserting direction for the QC Code chip. The QC Pouch contains one QC Code chip, which is used with the QC Cartridge to do instrument validation

# Maintenance


## FREND™ 2.0 Maintenance

5. When the QC Code chip installation is complete. Tap the **X** button to go to the setting screen.

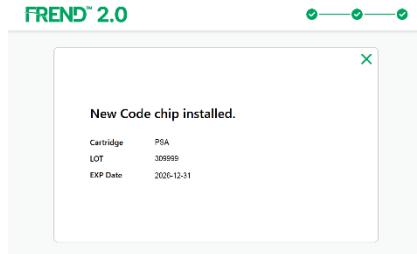

6. Tap the **ITEM** button on the setting screen.
7. Check the QC Cartridge lot number and the installed date.
8. If the QC Code chip installation is complete, tap the **← Back** button to go to the main screen.

9. Tap the **TEST** button on the main screen.

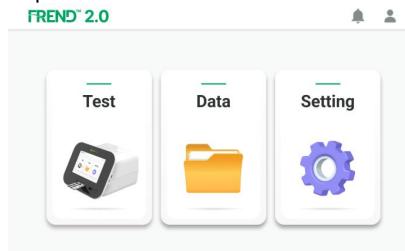


10. Tap the **Device QC** button on the TEST screen.



# Maintenance

## FREND™ 2.0 Maintenance


11. Insert the QC cartridge into the cartridge slot.

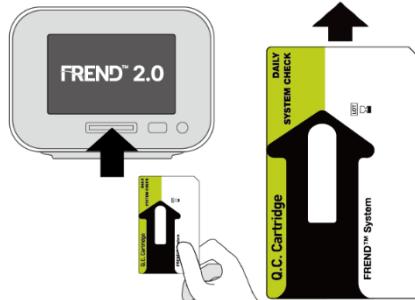

### **Warning:**

Please check the direction of the QC Cartridge before insertion.

12. The QC check that the instrument is operating correctly will complete automatically and the QC Cartridge will be expelled.

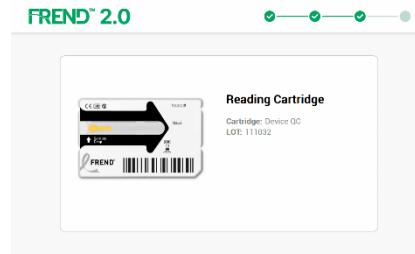

The system automatically checks three steps while reading.

- Step1.** Laser power
- Step2.** Laser alignment
- Step3.** Calculate ratio

13. When the QC check is done, the QC Cartridge automatically emerges and the results from all the three steps are displayed. There will be three Passes, if the system is properly operating.

### **Warning:**


If all results is not pass, try steps 9-12 again. If the device does not pass all three steps, please contact customer support via email.

# Maintenance

## FREND™ 2.0 Maintenance

14. Tap the **X** button and move to the main screen.

15. Remove the QC Cartridge.

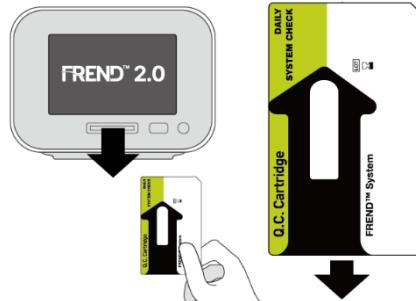


The FREND™ 2.0 setup is complete.


## FREND™ 2.0 Update

1. Tap the **SETTING** button on the main screen and select the **SYSTEM** button.

2. Connect the **USB drive** with update file to a USB port on the side and back of the device.

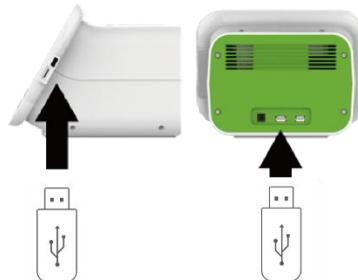

3. Tap the **OK** button to proceed with the SW update.

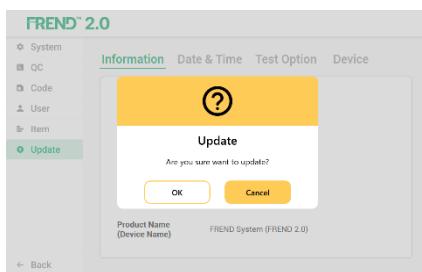

# Maintenance

## Cleaning and storage


- Do not clean the FREND™ 2.0 with strong or caustic cleansing agents, chemicals or cleansing tissues impregnated with chemicals.
- Use a soft and dry cloth to clean the FREND™ 2.0.
- For safety reasons, disconnect the power supply from the main outlet and remove the power adapter device from the FREND™ 2.0.
- If you want to store for a lengthy period, keep the FREND™ 2.0 covered in a dry place.
- Do not expose the device to direct sunlight.
- Recommended storage conditions are as follows:
  - Temperature: 15 ~ 30 °C
  - Humidity: 10 ~ 80 %
- Store the device on a stable surface. Avoid inclination, vibration and impact.
- Do not place the device near chemicals and/or corrosive substances.
- Keep the device, cable and other accessories well-organized.
- Maintain device cleanliness for its next use.
- Operate the device by lifting it cautiously and placing it down gently to prevent any impact.
- Refrain from placing heavy materials on the device.
- In storage, envelop or shield the device to safeguard it from dust.

# Maintenance

## Trouble-shooting

If the FREND™ 2.0 malfunctions, please check the following before you contact Customer Support.

### Error window on the FREND™ 2.0

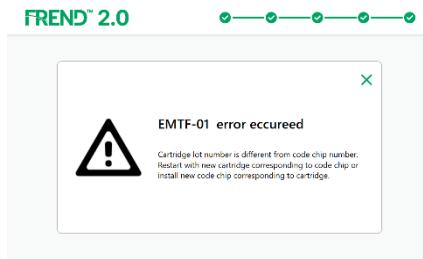

### Error list

#### ■ Cartridge insertion issues

Error code	Cause	Solution
EMCI-01	You did not insert the cartridge in 30 seconds.	Insert the cartridge.
EMCI-02	The motor started to run after inserting the cartridge, but it was not fully inserted.	Insert the cartridge completely.
EMCI-03 EMCI-04	The cartridge is inserted upside down or reversed.	Re-insert the cartridge correctly. After insertion, check to make sure the cartridge is properly and correctly inserted.

#### ■ Barcode issues

Error code	Cause	Solution
EMBR-01	The barcode printed on the cartridge may have been damaged so the reader is unable to interpret the code correctly.	Manually enter the LOT number of the cartridge using the keypad or replace it with a new one.
EMBR-02	The barcode information related to the cartridge lot number printed on the cartridge is not readable by the system reader.	Carefully enter the lot number of the cartridge again. If the same message is repeated, check the lot number on the installed code chip.
EMBR-03	The lot number entered for the cartridge does not match the lot number on the code chip.	Carefully enter the lot number of the cartridge again. If the same message is repeated, check the lot number on the installed code chip.

# Maintenance

## Trouble-shooting

### ■ Update issues

Error code	Cause	Solution
EMUF-01	There is no executable file on the USB drive. `	Save the executable file, "Frend2Update_X.X.X.fndpkg", transfer it to the USB drive and then retry the update process.
EMUF-02	Update failed during the process.	The update file may be damaged. Try again with using a new flash drive and update file.

### ■ Data backup issues

Error code	Cause	Solution
EMDB-01	Update failed during the process	Please check whether the flash drive meets the requirements of the FREND™ 2.0. Also, ensure that the flash drive is properly connected to the device.
EMDB-02	A problem has been detected when attempting to transfer data from the FREND™ 2.0 to the USB drive.	Check the connection of the USB port and USB. If the same problem occurs, contact your dealer or the manufacturer.

### ■ Data save issues

Error code	Cause	Solution
EMDS-01	The storage capacity of the FREND™ 2.0 to store the data has been exceeded.	Back up the data stored in the FREND™ 2.0 to a USB drive. Then, delete the data stored in the FREND™ 2.0.

### ■ Code chip install issues

Error code	Cause	Solution
EMCC-01	The code chip is not inserted properly.	Make sure that the code chip is inserted correctly in the direction of the arrow and push the code chip in until it sounds 'click'.
EMCC-02	The FREND™ 2.0 does not recognize the code chip.	Check that the code chip is correctly inserted, and restart the code chip installation. If the same problem occurs, contact your dealer or the manufacturer.

# Maintenance

## Trouble-shooting

### ■ Test result issues

Error code	Cause	Solution
EMTF-01	The lot number of the inserted cartridge is different from the lot number of the installed code chip.	Check that the lot number printed on the cartridge is the same as the lot number on the code chip. If not, restart using a code chip and cartridge of the same lot number.
EMTF-02	Unable to output a test result because the reference signal is weaker than the baseline.	Load the same sample into a new cartridge and insert the cartridge into the system. If the problem is repeated, try a sample from a different source (different patient). If the problem continues, contact your dealer or the manufacturer.
EMTF-03	Unable to output a test result because the reference signal is stronger than the baseline.	Load the same sample into a new cartridge and insert the cartridge into the system. If the problem is repeated, try a sample from a different source (different patient). If the problem continues, contact your dealer or the manufacturer.
EMTF-04	The system cannot detect any signal.	The sample may not be loaded or the sample may not be flowed due to air bubbles. After checking, restart the test with the new cartridge.
EMTF-05	The system detects more than five signals.	Foreign substance (dust) inside the cartridge may cause unintentional signals. Restart the test with the new cartridge. If the same problem occurs, contact your dealer or the manufacturer.
EMTF-06	The lateral flow of the sample within the cartridge is incomplete.	Check if there is insufficient sample volume, air bubbles in the sample, whether the pipette is defective, or if the specimen is loaded in the wrong place.
EMTF-07	The lateral flow is not completed after the specified time. (Time-out error)	Check if there is insufficient sample volume, air bubbles in the sample, whether the pipette is defective, or if the specimen is loaded in the wrong place.
EMTF-08	The cartridge has passed the expiration date.	Load the sample into a new cartridge which does not pass the expiration date and restart the test.

### ■ Test mode matching issues

Error code	Cause	Solution
EMMF-01	Different type of cartridge is read in QC Cartridge Mode	Read QC Cartridge in QC Cartridge Mode.
EMMF-02	QC Cartridge is read in the different mode	Use the QC Cartridge in the designated Mode.

# Maintenance

## General specification –normal environmental conditions

<b>Electrical rating</b>	Voltage AC 100 -240 , 1.7A Frequency 50 / 60 Hz
<b>Electric input (Adaptor)</b>	Voltage DC 12 V Current 5.0 A
<b>Dimensions</b>	276 mm x 263 mm x 202 mm (W x L x H) 10.9 inch X 10.3 inch X 7.9 inch
<b>Weight</b>	3.4kg (7.5 lb.)
<b>Optical Power (Laser)</b>	Class 1 laser product (IEC 60825-1:2014) Wavelength 635 nm CW Out Power Max. 25 mW
<b>User interface</b>	Active screen size 8.0 inches diagonal dimension Pixel format 1920 x 1080, Capacitive Touch
<b>Printer</b>	Printing speed 50 mm/sec
<b>Environmental suggestions for optimal performance</b>	<p>Do not place the unit in direct sunlight.</p> <p>Position the unit in a well-ventilated area.</p> <p>Place the unit on a flat, dry and smooth surface with sufficient ventilation area around the unit.</p> <p>Operating condition: Temperature: 10 ~ 40 °C, Humidity: 10 % ~ 80 %</p> <p>Storage condition: Temperature: 10 ~ 40 °C, Humidity: 10 % ~ 80 %</p>

### Installation Condition

- 1.1 Indoor use (For outdoor use, a protective case must be manufactured and attached inside to use)
- 1.2 Altitude : 2,000m or less
- 1.3 Ambient temperature : 10 ~ 40 degrees or less (When used outdoors, the temperature control device inside the protective case should be designed to be within the appropriate temperature range)
- 1.4 For a temperature below 31°C, which decreases linearly from an ambient temperature of 40°C to a relative humidity of 50%, the maximum relative humidity should be 80%
- 1.5 Mains supply voltage fluctuations Nominal voltage must be less than  $\pm 10\%$
- 1.6 Transient overvoltage should be below the overvoltage category I
- 1.7 Temporary overvoltage from mains supply equipment
- 1.8 The degree of pollution in the intended condition (in most cases, the degree of pollution is 2)

# Maintenance

## Customer support information

Henceforth, please be aware that all materials in this manual are safeguarded by Korean and international copyright laws. Reproduction, translation, publication, or distribution without the permission of the copyright owner is strictly prohibited.

With every endeavor made to prevent errors in text and diagrams, please note that NanoEntek Inc. does not accept responsibility for any inadvertent errors that may arise in this publication. The information and specifications provided in this document are subject to modification without prior notice. For the most current information, kindly reach out to NanoEntek, Inc.'s customer support.

As this product is distributed globally, please be aware that customer support services differ based on geographical regions. Upon shipping the FREND™ 2.0, you will receive information containing the relevant telephone numbers, fax numbers, and email addresses for obtaining support specific to your geographical region.

Notwithstanding the careful review of the information in this manual, it should be noted that the copyright owner reserves the right to make changes without prior consent or notification, even though it has been verified for accuracy.

Copyright © 2025 by NanoEntek, Inc.  
All rights reserved. Published in Korea.

# FREND™ 2.0

NESMU-F20-001EN (V.0.0)



**NanoEntek, Inc.**

851-14, Seohae-ro, Paltan-myeon, Hwaseong-si  
Gyeonggi-do, 18531, Korea  
Tel: +82-2-6220-7940 / Fax: +82-2-6220-7999

**US Corporation**

**NanoEntek America, Inc.**

220 Bear Hill Road, Suite 102, Waltham, MA 02451, USA  
Tel: +1-781-472-2558 / Fax: +1-781-790-5649

**European Corporation**

**NanoEntek Europe I med-tech supplies GmbH**

Lochhamerstr. 4a, 82152 Martinsried, Germany  
Tel: +49-89-21-55-38-43 / Fax: +49-89-99-95-46-60

**EC REP**

**MT Promedt Consulting GmbH**

Ernst-Heckel-Straße 7, 66386 St. Ingbert, Germany

**UK Representative**

**MT Promedt Consulting Ltd.**

First Floor, Park Central, 40-41 Park End Street  
Oxford OX1 1JD, United Kingdom

**E-mail**

ivdst@nanoentek.com

**Website**

www.nanoentek.com